

BioLINE Allergy Reagent Kit

(Immunoblotting)

REF

MB0000275; MIX-20, D; 24 Tests/kit
MB0000284; MIX-16, D1; 24 Tests/kit
MB0000285; INH-10, D2; 24 Tests/kit
MB0000286; FD-8, D3; 24 Tests/kit
MB0000287; MIX-12, D4; 24 Tests/kit

INTENDED USE

BioLINE Allergy Reagent Kit (D), is an in vitro semi quantitative assay for the determination of allergy specific IgE to multiple allergens.

Allergens include Cross-reactive carbohydrate Determinant/Dermatophagoides

pteronyssinus/Dermatophagoides farinae/Cat
dander/Dog dander /Egg
white/Peanut/Soybean/milk/Crab/Shrimp/Beef/Fish/
Scallop/ Carp/Salmon/Bass black/Lobster
/Mutton/House dust mite/Cockroach, German
/Penicillium chrysogenum/Cladosporium
herbarum/Aspergillus fumigatus /Alternaria alternata
/Willow/Cottonwood/Elm/Common ragweed
/Japanese Hop /Mugwort.

It is intended for in vitro diagnostic use as an aid in the clinical diagnosis of IgE mediated allergic disorders in conjunction with other clinical findings, and is to be used in clinical laboratories for professional use.

SUMMARY&EXPLANATION OF TEST

Immunoglobulin class E was discovered in 1966 by the Japanese scientist couple Teruko and Kimishige Ishizaka. It plays an essential role in Type I hypersensitivity. There are over 15% people suffering from Type I allergic reaction in industrialized country. In allergic patients, they will have multiple syndromes, such as dermatitis, rhinitis, hay fever, asthma, edema, diarrhea, and pruritus. This assay provides visual detection of allergen-specific IgE in human serum. The detection of increased amounts of circulating allergen specific IgE, when interpreted in context with allergic history and physical examination, can contribute to the diagnosis and assessment of IgE-mediated allergic diseases.

PRINCIPLES OF THE PROCEDURE

The kit adopts immunoblotting to detect allergen specific IgE antibody in human serum. IgE antibodies in the sample bind to the corresponding allergens which are coated on nitrocellulose membranes to make the IgE antibody in serum combined with the corresponding reaction zone on the test strip. After washing, biotinylated mouse anti human IgE antibodies are added for incubation. After washing again, alkaline phosphatase-labeled Streptavidin are added to form mouse anti human IgE antibody-IgE antibody-biotinylated mouse anti human IgE antibody alkaline phosphatase-labeled streptavidin complex or allergen-specific IgE antibody -biotinylated mouse anti human IgE antibody alkaline phosphatase-labeled streptavidin complex.

The strip is then washed again to remove any unbound SA-AP. After addition of the substrate solution for incubation, the alkaline phosphatase fixed on the membrane strip by the above complex catalyzes the substrate reaction. Visual blue-purple color change will be observed which indicates the existence of specific IgE antibodies against respective allergens.

After the reaction, the reaction was terminated with purified water, and the gray value of the reaction area was read after drying. The gray value is proportional to IgE amount.

WARNINGS AND PRECAUTIONS

- Package insert instructions must be followed accordingly. Reliability of assay results cannot be guaranteed if there are any deviations from the instructions in this package insert.
- For professional in vitro diagnostic use only.
- For single use only. Do not re-use.
- The instruments used shall be routinely checked to ensure correct operation within their functional range
- Do not use reagents beyond the expiration dates.
- The kit contains human sourced materials. All recommended precautions for the handling of blood derivatives should be taken. Please refer to the OSHA Standard on Blood borne Pathogens or Biosafety Level ¹⁰ or other appropriate biosafety practices. ^{11,12}
- Do not swallow the reagents. Avoid contact with

eyes, skin and mucous membranes. All patient specimens should be handled as potentially infectious. Wear protective clothing and disposable gloves according to Good Laboratory Practices.

- Liquid waste and solid waste should also be handled in accordance with the appropriate biosafety practices same as stated above.



Precautions

- The solutions contain ProClin300 $\leq 0.1\%$ as preservative and surfactant and may cause an allergic skin reaction by skin contact. Avoid contact with skin. Wear protective gloves, protective clothing and take eye protection.
- Any serious incident that has occurred in relation to the device shall be reported to the manufacturer and the competent authority of the Member State in which the user and/or the patient is established.

MATERIALS PROVIDED

- **Strips** coated with the corresponding allergens on nitrocellulose membranes, ready to use.
 -1 X 24 strips for 24T; **STRIP**
- **Sample Diluent** 0.5% BSA in 0.05M Tris buffer, ready to use.
 -1 X 60 mL for 24T; **DIL**
- **Biotinylated Anti-IgE antibodies** consisting of 0.2 μ g/mL~0.8 μ g/mL biotinylated anti-human-IgE in 0.05M Tris buffer, ready to use.
 -1 X 40 mL for 24T; **Anti-IgE** **BIOT**
- **Streptavidin Conjugate** consisting of 1:2000~1:8000 streptavidin AP conjugate in 0.05M MES buffer, ready to use.
 -1 X 40 mL for 24T; **CONJ**
- **Substrate** light yellow liquid, consisting of NBT/CBIP, ready to use.
 -1 X 40 mL for 24T; **SUBS**
- **Wash Buffer concentrate** transparent liquid, consisting of a 10X concentrate in 0.05M Tris buffer, pH7.5 $\pm$ 0.2.
 -1 X 50 mL for 24T; **BUF** **WASH** **10x**
- **Scoring Sheet**
 -1pc for 24T;
- **Incubation Tray**
 -3pcs for 24T;


MATERIALS REQUIRED BUT NOT PROVIDED

- Distilled or de-ionized water **H₂O** **DIST**
- Shaker
- Timer
- Pipette (200-1000 μ L)
- Absorbent paper
- Latex gloves


Illustration of Panel allergen and test strip

No.	CODE	ALLERGEN
1	CCD	Cross-reactive carbohydrate Determinant
2	D1	Dermatophagoides pteronyssinus
3	D2	Dermatophagoides farinae
4	E1	Cat dander
5	E5	Dog dander
6	F1	Egg white
7	F13	Peanut
8	F14	Soybean
9	F2	milk
10	F23	Crab
11	F24	Shrimp
12	F27	Beef
13	F3	Fish
14	F338	Scallop
15	F355	Carp
16	F41	Salmon
17	F65	Bass black
18	F80	Lobster
19	F88	Mutton
20	H1	House dust mite
21	I6	Cockroach, German
22	M1	Penicillium chrysogenum
23	M2	Cladosporium herbarum
24	M3	Aspergillus fumigatus
25	M6	Alternaria alternata
26	T12	Willow
27	T14	Cottonwood
28	T8	Elm
29	W1	Common ragweed
30	W22	Japanese Hop
31	W6	Mugwort


Model I

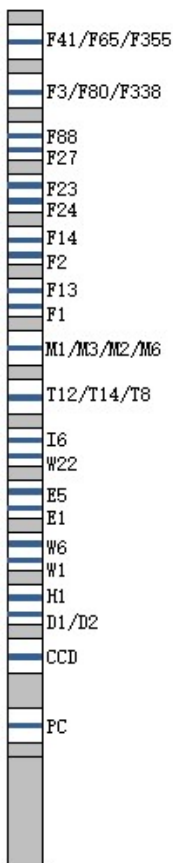


Model II

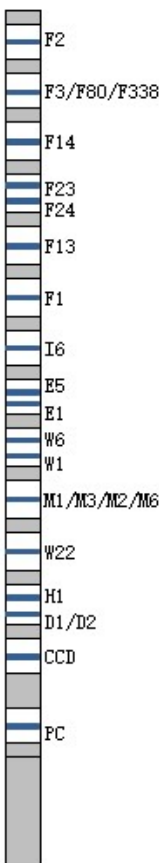


Model III

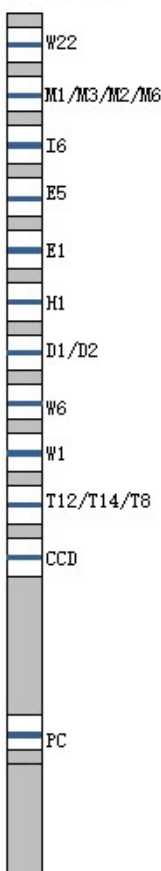

Model IV

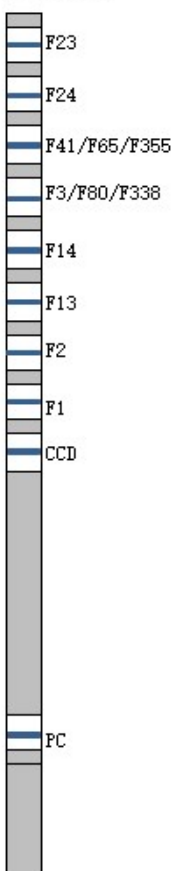

Model V

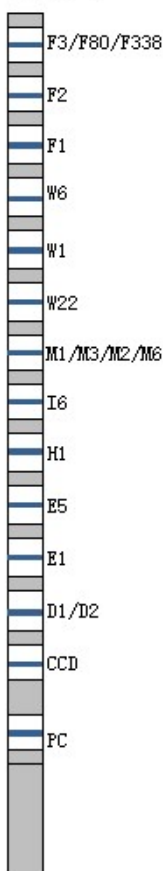

REAGENT PREPARATION AND STORAGE

- Store the kit at 2-8 °C. The shelf life of the

unopened kit is 18 months. Do not freeze any components.

- Vial opened reagents could be used for 28 successive days stored at 2-8°C. Used vials should be closed carefully and stored at 2-8°C.
- Do not use components beyond the expiration date.
- Do not combine reagents of other suppliers or kit components with this kit.
- Substrate Solution is light sensitive reagent and avoids exposing this reagent to illumination. Do not use Substrate Solution if it gets turbid or blue.
- To avoid potential microbial and/or chemical contamination, unused reagents should never be transferred into the original vials.
- Do not interchange caps of kit components.
- Do not use reagents and test strips with broken package.

Wash Buffer 10X Concentrate

Dilute one part with nine parts distilled or de-ionized (D.I.) water. Diluted wash buffer is stable for 6 weeks stored at 2-8°C. Any crystallized salt inside the bottle must be resolved before use.

RCNS	H2O
------	-----

SPECIMEN COLLECTION, STORAGE AND HANDLING

- Serum from venous only can be used.
- Serum which is collected according to standard procedure is stable for 2 days at 2-8°C and may be frozen at or below -20°C for longer time.
- Before testing, the frozen samples shall be thawed at room temperature (20-25°C), gently reversed and mixed evenly. Avoid repeated freezing and thawing.
- Do not use 56°C heat inactivated samples.
- Sera with interfering substances (hemolysis, blood lipid or jaundice) are not recommended to be tested by this assay.
- The samples don't need to be diluted, ready to use.

ASSAY PROCEDURE

Reagent Preparation

- | | |
|---|---------------|
| Sample Diluent | ready to use. |
| Biotinylated Anti-IgE antibodies | ready to use. |
| Streptavidin Conjugate Solution | ready to use. |
| Substrate Solution | ready to use. |

Wash Buffer 10X concentrate

Dilute one part with nine parts distilled or de-ionized (D.I.) water. Diluted wash buffer is stable for 1 weeks stored at room temperature.

ASSAY PROCEDURE

- Please shake test strips at room temperature with gentle agitation during all incubation steps. If the temperature is too high or too low, the results will not be within the quality control range.
- Washing steps are very important. Incorrect washing will lead to wrong results.
- In order to avoid cross contamination and false positive results, it is recommended to use the correct suction method.

Manual operation

1. Allow the test kit and all its components to reach room temperature before use. (no less than 30 minutes is recommended)
2. Put test strip into the incubation tray, each incubation tray carries one strip. Unused strips should be sealed into the aluminum pouches together with desiccant.
3. Add 1000 μ L of Sample Diluent into each incubation tray.
4. Incubate the test strip for 5 minutes at room temperature (20-25°C) with gentle agitation, and then remove it.
5. Add 800 μ L of Sample Diluent into each incubation tray, then pipette 200 μ L of patient sample and add it into the incubation tray.
6. Incubate for 25 minutes at room temperature (20-25°C) with gentle agitation.
7. Remove diluted samples completely. Wash test strip 3 times using 1500 μ L Wash Buffer for 1 minutes with gentle agitation. Remove Wash Buffer after every washing step.
8. Pipette 1000 μ L Biotinylated Anti-IgE antibodies.
9. Incubate for 20 minutes at room temperature (20-25°C) with gentle agitation. Remove

Biotinylated Anti-IgE antibodies. Repeat washing steps of step 7.

10. Pipette 1000 μ L Conjugate Solution and incubate for 10 minutes at room temperature with gentle agitation. Remove Conjugate. Repeat washing steps of step 7.
11. Add 1000 μ L Substrate Solution and incubate for 15 minutes at room temperature (20-25°C) with gentle agitation.
12. Remove Substrate. Wash with 1000 μ L distilled or de-ionized (D.I.) water for 1 minute at room temperature (20-25°C) with gentle agitation. Repeat this wash step for another 2 times.
13. Dry test strip, and stick it onto the Scoring Sheet to record the test results.
14. Judge the specific IgE level of the sample according to the gray value with the interpretation system.

Operation by automatic immunoblotting instrument

Detailed information about operation can be taken from the Instrument User's Manual.

Note that, it is important to perform all routine maintenance procedures for optimal performance.

1. Put the reagents into the corresponding position of the reagent chamber of the fully automatic immunoblotting analyzer and empty the waste liquid bottle.
2. Turn on the power supply of the analyzer and start the operation program of the automatic immunoblotting analyzer.
3. Put the test strip into the corresponding slot of the analyzer. place the sample to be tested in the sample chamber, edit the sample information, select the item and perform the test.
4. The test results are automatically executed by the system.
5. After the experiment, the sample and reagent shall be recovered and the pipeline shall be flushed.

QUALITY CONTROL PROCEDURES

A control line is provided on each test strip. The test result is valid if a visible control line is presented.

CUT-OFF VALUE DETERMINATION

Clinical significance cut-off of allergen-specific IgE concentration has been set at 0.35 IU/mL for indication for sensitization.

Through the evaluation of 200 clinical samples, the concentration value of clinical samples was analyzed by receiver operating characteristic curve (ROC curve), which confirmed the rationality of the cut off value.

Note: Each laboratory shall determine the usability of cut-off value through experiments. If necessary, it is recommended that each laboratory establish its own cut-off value.

INTERPRETATION OF RESULTS

For each allergen, the coloring intensity on the membrane strip (gray value) is directly proportional to the content of specific IgE antibody in the patient's serum.

Score the test results according to the coloring intensity of the strip as Class 0-6. The test result is negative for a given allergen if no band is to be recognized, designated as Class 0. The test result is positive for a given allergen if a band exhibits a staining, and based on different coloring intensities, designated as Class 1-6.

IU/mL	Class	Allergen-specific IgE content
<0.35	0	None or hardly any found
0.35-0.69	1	Low
0.7-3.49	2	Increased
3.5-17.49	3	Significantly increased
17.5-49.9	4	High
50-100	5	Very high
>100	6	Extremely high

The positive results of mixed allergens show that the specific IgE antibodies of one or more allergens are positive. When it is necessary to further determine the single allergen specific IgE antibody concentration, it is recommended to use an appropriate single allergen specific IgE antibody detection kit for re-detection. The single detection concentration is not comparable to the mixed item detection

concentration, and the mixed item detection concentration cannot be considered as the sum of single concentrations.

PERFORMANCE CHARACTERISTICS

- Appearance and volume:** The outer package box shall be clean and tidy, label shall be clear and accurate. Each component in the kit shall be complete. Reagent bottle sealed no leakage and the liquid shall be clear and transparent. The strip shall be clean, free of stain and damage.
- Coincidence rate of negative reference materials:** The coincidence rate of negative reference materials shall be 100%.
- Coincidence rate of positive reference materials:** The coincidence rate of positive reference materials shall be 100%.
- Detection limit:** The detection limit shall not be greater than 0.35 IU / ml.
- Correlation:** Test the reference panel, the difference of a certain sample result should not be more than one class in the same direction. The result of positive samples should not be negative and the result of negative samples should not be positive.
- PRECISION:**
INTRA-ASSAY: Two repeatability references (weak positive and positive) were taken and tested with 10 replicates for each in a single run. Coefficient of variation (CV) was calculated for each of two samples. CV≤15%.
INTER-ASSAY: Two repeatability references (weak positive and positive) were taken and tested with 4 replicates in a single run, 2 runs per day for 10 days. Coefficient of variation (CV) was calculated for each of two samples. CV≤15%.
- METHOD COMPARISON:** Method comparison was implemented by comparing the clinical samples results of the assay to the results of predicated assay. The positive and negative agreement were analyzed, sensitivity and specificity were summarized. Sensitivity ≥ 85%, specificity ≥ 90%.
- Interference:** No interference has been observed on negative reference and detection limit reference with bilirubin, hemoglobin, triglycerides at the level indicated below: Hemoglobin ≤ 400 mg/L; Bilirubin ≤ 20 mg/dL; Triglycerides ≤ 2,000 mg/dL.

TEST LIMITATIONS

1. A negative result indicates the absence of circulating IgE to the test allergen, suggesting that symptoms may be due to other causes. However, a negative result does not exclude clinical sensitivity since some individuals may elicit negative test results in the presence of clinical allergy. Allergic hypersensitivity reactions to altered, (e.g. by industrial processing, cooking or digestion) or related food allergens may be also be present, therefore caution should be taken in further investigative procedures.
2. A positive result must be used in associated with clinical evaluation and diagnostic procedures. The values obtained from this assay are intended to be an aid for IgE-mediated allergic disease diagnosis only.

SYMBOLS

	Catalog Number		Use-by date
	In Vitro diagnostic medical device		Lot Number
	Store between +2°C and +8°C		Consult Instruction for Use
	Manufacturer		Authorized Representative in the European Community
	CE Marking		Contains Sufficient for <n> Tests
	Biological Risk		GHS07 Warning

		Biotinylated allergen
---	---	-----------------------

REFERENCES

1. Sanchez-Velasco P, Mendizabal L, Anton E M, et al. Association of hypersensitivity to the nematode *Anisakis simplex* with HLA class II DRB1*1502-DQB1*0601 haplotype. Hum Immunol, 2000; 61:314-319.
2. Johansson, S.G., H.H.Bennich, et al. The clinical significance of IgE. Progress in Clin Immunol, 1972; 1:157-81.
3. Torres-Galvan M J, Quiralte J, Blanco C, et al. Linkage of house dust mite allergy with the HLA region. Ann Allergy Asthma 5 Immunol, 1999; 82:198-203.
4. Kleine-Tebbe J, Breuer K, Lepp U, et al. Spezifische IgE-werte gegen aero- und nahrungsmittelallergene

im vergleich: Dr. Fooke ALLERG-O-LIQ und Pharmacia CAP-System. Allergologie 2004; 4:129-134.

5. Bertout S, Badoc C, Mallie M, et al. Spore diffusate isolated from some strains of *aspergillus fumigates* inhibits phagocytosis by murine alveolar macrophages. FEMS Immunol Med Microbiol, 2002; 33:101.
6. Klink M, Cline MG, Halonen M, Burrows B. Problems in definig normal limits for serum IgE. J Allergy Clin Immunol, 1990; 85: 440-444.
7. Thomas L. Labor und Diagnose. 4. Auflage, Medizinische Verlagsgesellschaft, Marburg 1992.
8. Barbee RA, Halonen M, Kaltenborn W, Lebowitz M, Burrows B. A longitudinal study of serum IgE in a community cohort: Correlations with age, sex, smoking, and atopic status. J Allergy ClinImmunol, 1987; 79: 919-927.
9. US Department of Labor, Occupational Safety and Health Administration, 29 CFR Part 1910.1030, Occupational Exposure to Bloodborne Pathogens.
10. US Department of Health and Human Services. Biosafety in Microbiological and Biomedical Laboratories, Fourth Edition. Washington, DC: US Government Printing Office, May 1999.
11. World Health Organization. Laboratory Biosafety Manual. Geneva: World Health Organization; 2004.



HOB Biotech Group Corp., Ltd.
C6 Building, No. 218 Xinghu Road, Suzhou Industrial Park,
Suzhou, Jiangsu, 215123, China

CONTACT INFORMATION:

TEL (+86)512-69561996

Fax (+86)512-62956652

WEBSITE: www.hob-biotech.com

CUSTOMER SERVICE: TEL (+86)4008601202



EUROPE REPRESENTATIVE: Emergo Europe

ADDRESS/LOCATION:

Prinsessegracht 20, 2514 AP The Hague, The Netherlands



The eIFU is available on Website:

<http://en.hob-biotech.com/usercenter/login.aspx>

TECHNICAL ASSISTANCE

For technical assistance, contact your National Distributor.

Date of issue: 2022-01-20

Version: A/0 (EN)